

BREAST CANCER ANTIGEN (CA15-3)

INTENDED USE

The CA 15-3 EIA test is intended for use as a monitoring and screening test for breast cancer. An abnormal result (i.e., elevated serum CA15-3 level) indicates further clinical management. CA 15-3 is a useful tumor marker for patients in clinical remission following treatment. Post-operative serum CA 15-3 values which fail to return to normal, strongly suggest the presence of residual tumor, while tumor recurrence is often accompanied by a rise of serum CA 15-3 before progressive disease is clinically evident.

INTRODUCTION

Breast cancer is the most common life-threatening malignant lesion in women of many Developed countries today, with approximately 180,000 new cases diagnosed every year. Roughly half of these newly diagnosed patients are node-negative, however 30% of these cases progress to metastatic disease.

There are a number of tumor markers that can help clinicians to identify and diagnose which breast cancer patients will have aggressive disease and which will have an indolent course. These markers include estrogen and progesterone receptors, DNA ploidy and percent-S phase profile, epidermal growth factor receptor, HER-2/neu oncogene, p53 tumor suppressor gene, cathepsin D, proliferation markers and CA 15-3. CA 15-3 is most useful for monitoring patients post-operatively for recurrence, particularly metastatic diseases. 96% of patients with local and systemic recurrence have elevated CA 15-3 which can be used to predict recurrence earlier than radiological and clinical criteria. A 25% increase in the serum CA 15-3 is associated with progression of carcinoma. A 50% decrease in serum CA 15-3 is associated with response to treatment. CA 15-3 are more sensitive than CEA in early detection of breast cancer recurrence. In combination with CA-125, CA 15-3 has been shown to be useful in early detection of relapse of ovarian cancer. CA 15-3 levels are also increased in colon, lung and hepatic tumors.

TEST PRINCIPLE

The CA15-3 EIA test is a two-site solid phase enzyme immunoassay. The molecules of CA15-3 are "sandwiched" between two monoclonal antibodies. One coated to the bottom of the wells of the microtiter plates and the other linked to the horseradish peroxidase (enzyme conjugate). After incubation and washing, the enzymatic reaction develops a color which is proportional to the amount of CA15-3 molecules present in the assay.

MATERIALS AND COMPONENTS

Materials provided with the test kits:

1. Monoclonal Anti-CA15-3 antibody coated microtiter plate with 96 wells.
2. Sample diluent, 100ml
3. Enzyme conjugate reagent, 12ml
4. CA 15-3 reference standard set, containing 0, 15, 30, 60, 120, and 240 Unit/ml (liquid, ready for use) or lyophilized form.
5. Wash Buffer Concentrate (50X), 15 ml.
6. TMB substrate, 12 ml
7. Stop solution, 12ml

Materials required but not provided

1. Precision pipettes and tips, 0.1ml, 0.2ml, 1ml and 5ml.
2. Distilled water.
3. Disposable pipette tips.
4. Vortex mixer.
5. Absorbent paper or paper towel.
6. A microtiter plate reader at 450nm wavelength, with a bandwidth of 10nm or less and an optical density range of 0-2. OD or greater.
7. Graph paper.

SPECIMEN COLLECTION AND PREPARATION

1. Blood should be drawn using standard venipuncture techniques and the serum should be separated from the red blood cells as soon as practical. Avoid grossly hemolytic, lipemic or turbid samples.
2. Plasma samples collected in tubes containing EDTA, heparin, or oxalate may interfere with test procedures and should be Avoided.
3. Specimens should be capped and may be stored for 48 hour at 2-8°C prior to assaying. Specimens held for a longer time can be frozen at -20°C for 6 months prior to assaying. Thawed samples should be inverted several times to mix prior to testing.

STORAGE OF TEST KITS AND INSTRUMENTATION

1. Unopened test kits should be stored at 2-8°C upon receipt and the microtiter plate should be kept in a sealed bag with desiccants to minimize exposure to damp air. The test kit may be used throughout the expiration date of the kit refer to the package label for the expiration date.
2. Opened test kits will remain stable until the expiring date shown provided it is stored as prescribed above.
3. A microtiter plate reader with a bandwidth of 10nm or less and an optical density range of 0-2 OD or greater at 450nm wavelength is acceptable for use in absorbance measurement.

REAGENT PREPARATION

1. All reagents should be brought to room temperature (18-25°C) before use. All reagents should be mixed by gently inverting or swirling prior to use. Do not induce foaming.
2. If reference standards are lyophilized, reconstitute each standard with 0.5ml distilled water. Allow the reconstituted material to stand for at least 20 minutes. Reconstituted standards should be sealed and stored at 2-8°C.
3. Dilute 1 volume of Wash Buffer (50x) with 49 volumes of distilled water. For example, dilute 15ml of wash buffer concentrate (50X) into 735ml of distilled water to prepare 750ml of washing buffer (1x). Mix well before use.

ASSAY PROCEDURE

Important Note:

The CA15-3 standards have already been prediluted and are ready for use.

PLEASE DO NOT DILUTE AGAIN

1. Patient serum and control serum should be diluted, 51 fold, before use. Prepare a series of small tubes (such as 1.5ml microcentrifuge tubes) and mix 20µl serum with 1.0ml sample diluent.
2. Secure the desired number of coated wells in the holder, dispense 100 µl of CA15-3 standards diluted specimens and diluted controls into the appropriate wells. Gently mix for 10 seconds.
3. Incubate at 37°C for 1 hour.
4. Remove the incubation mixture by emptying the plate content into a waste container. Rinse and empty the microtiter plate 5 times with 1x wash buffering. Strike the microtiter plate sharply onto absorbent paper or paper towels to remove all residual water droplets.
5. Dispense 100 µl of enzyme conjugate reagent into each well. Gently mix for 10 seconds.
6. Incubate at 37°C for 1 hour.
7. Remove the contents and wash the plate as described in step 4 above.
8. Dispense 100 µl TMB substrate reagent into each well. Gently mix for 10 seconds.
9. Incubate at room temperature in the dark for 20 minutes.
10. Stop the reaction by adding 100 µl of stop solution to each well. Gently mix for 10 seconds ensuring that the blue color completely changes to yellow.
11. Read the optical density at 450nm with a microtiter plate reader within 15 minutes.

IMPORTANT NOTE

1. The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbance readings.
2. It is recommended that no more than 32 wells be used for each assay run, if manual pipetting is used, since pipetting of all standards, specimens and controls should be completed within 5 minutes. A full plate of 96 wells may be used if automated pipetting is available.
3. Duplication of all standards and specimens, although not required, is recommended.

CALCULATION OF RESULTS


Calculate the mean absorbance value for each set of CA15-3 reference standards, Specimens and controls. Construct a standard curve by plotting the mean absorbance

obtained from each reference standard against its concentration in units per ml on linear graph paper, with absorbance values on the vertical or Y axis and concentration on the horizontal or X axis. Use the mean absorbance values for each specimen to determine the corresponding concentration of CA15-3 in units per ml from the standard curve. It is recommended that samples be analyzed in duplicates. Since the CA15-3 standards have already been diluted 51-fold, there is no need for the samples or controls to be multiplied by the dilution factor.

EXAMPLE OF STANDARD CURVE

Results of typical standard run with optical density reading at 450nm shown in the X axis.

CA 15-3 VALUES (U/ml)	Absorbance (450nm)
0	0.021
15	0.425
30	0.693
60	1.214
120	1.956
240	2.845

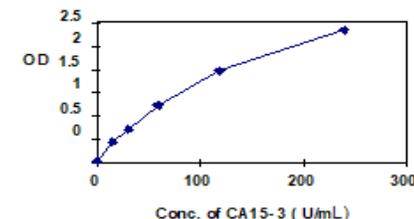

This standard curve is for the purpose of illustration only, and should not be used to calculate unknowns. Each user should obtain his or her own standard curve and data.

EXPECTED VALUES AND SENSITIVITY

Healthy women are expected to have CA15-3 values below 35 U/ml. The minimum detectable concentration of CA15-3 in this assay is estimated to be 5U/ml.

PERFORMANCE CHARACTERISTICS

1. **Accuracy:** Comparison between our assay and commercial available kits provide the following data
N = 55
Correlation Coefficient= 0.975
Slope = 0.924
Intercept = 1.92
Mean (Our Kits) = 28.93
Mean (Abbott) = 26.78
2. **Precision:**

1. Intra Assay				
Concentrations	N	Mean	S.D	%CV
Level	20	16.2	0.970	5.96
Level I	20	86.26	4.290	4.97

2. Inter-Assay				
Concentrations	N	Mean	S.D	%CV
Level	10	11.89	1.098	9.23
Level I	10	106.32	6.460	6.07

BREAST CANCER ANTIGEN (CA15-3)

3. Linearity

Two patient sera were serially diluted with 0 U/mL standard in a linearity study. The average recovery was 99%

SAMPLE A			
Dilution	Expected	Observed	% Recov.
Undiluted	180.81	180.81	
2x	90.41	88.92	98.4
4x	42.21	43.72	103.6
8x	22.60	23.03	101.9
16x	11.30	12.04	106.5
Average Recovery 102.6%			

SAMPLE B			
Dilution	Expected	Observed	% Recov.
Undiluted	207.19	207.19	
2x	103.60	105.23	101.6
4x	51.80	50.33	97.2
8x	25.90	26.67	103.0
16x	12.95	13.91	107.4
Average Recovery 102.3%			

PRESENTACIÓN:

CONT. 96 TEST CODIGO: RSET006

REFERENCES:

1. Aziz DC, Rittenhouse HJ, Ranken R. Use and interpretation of test in oncology. Santa Mónica: Specialty Laboratories, 1991.
2. Aziz DC, Quantitation of estrogen and progesterone receptors by immunocytochemical and image analyses. A J Clin Pathol 1992;98:105-11
3. Aziz DC, Peter JB. DNA ploidy and cell-cycle analysis. Tools for assessment of cancer prognosis. J Clin Pathol 1991;5:422-38.
4. Clark GM Dressler LG, Owens MA, Dounds G, Oldaker T, McGuire WL. Prediction of relapse or survival in patients with node-negative breast cancer by DNA flow cytometry. N Engl J Med 1989;320:627-33.
5. Elledge RM, McGuire WL. Prognostic factors and therapeutic decisions in axillary node-negative breast cancer. Annu Rev Med 1993;44:201-10.
6. Foekens JA, Rio C, Seguin P, et al. Prediction of relapse and survival in breast cancer patients by pS2 protein. Cancer Res 1990;50:3832-7.
7. Isola J, Visakorp T, Holli k, Kallioniemi D. Association of p53 Expression with other prognostic factors and long term Survival in node-negative breast cancer. J Cell Biochem 1992; /Suppl 16D): 101.
8. Kute TE, Shao ZM, Snugg NK, Long RT, Russel GB, Case LD. Cathepsin D as a prognostic indicator for node-negative Breast Cancer patients using both immunoassays and enzymatic assays. Cancer Res 1992;52:198-203.
9. McGuire WL, Tandon AK, Allred D Chamnes GC, Clark GM. How to use prognostic factors in axillary node Negative breast cancer patients. J Natl Cancer Inst 1990;82:1006-7.
10. Nicholson S, Richard J, Sainsbury C, et al. Epidermal growth factor receptor(EGFr): results of a 6 year follow up study in operable breast cancer with emphasis on the node-Negative subgroup. Br J Cancer 1991;63:146-50.
11. Somerville JE, Clarke LA, Biggart JD. C-ERB B-2 overexpression and histological type of in-situ and invasive Breast carcinoma. J Clin Pathol 1992;45:16-20.
12. Ueronese S, Gambacorta M. Detection of KI-67 rate in Breast Cancer. Am J Clin Pathol 1991;95:30-4.
13. Lotnick M, Pavesi F, Scarabelli M. Tumor associated Antigens CA15-3 and CA-125 in ovarian cancer. Int J. Biolog Markers 1991;6:115.